



Comfort Inception Cushion - Custom

HCPCS CODE: E2609

Customer information

Date: _____
Company name/ACCT #: _____
Name: _____
Weight: _____
Height: _____
Reference: _____

W/C manufacturer: _____
Model #: _____ Serial #: _____

For best results, do not fill out in your browser. Interactive form should be completed using *Adobe Reader* after saving to your local drive. Then email to orders.comfort@permobil.com or print and fax to 877.636.8944.

DO NOT SEND PROTECTED HEALTH INFORMATION. IT IS NOT NEEDED TO MAKE THE PRODUCT YOU ARE REQUESTING.

P.O. number: _____

Requested by: _____

Phone: _____ Fax: _____

Email: _____

Ship to: _____

Additional information: _____

1 Size, cover, & shape

1.1 Size

Custom part number:

C-C- W D

Please fill in the above with desired dimensions
or select a size in the chart below.

Example part number: **C-C-15W18D**

*If desired size is not listed below, a 60%
upcharge will be applied for materials and
Customer Support approval is required.

Base MSRP by size

Depth																																																				
	10"	11"	12"	13"	14"	15"	16"	17"	18"	19"	20"	21"	22"	23"	24"	25"	26"	27"	28"																																	
22"	\$523.00																								\$1,000.00																											
21"																																																				
20"																																																				
19"																																																				
18"																																																				
17"	\$397.00												\$498.00																																							
16"																																																				
15"																																																				
14"																																																				
13"																																																				
12"																																																				
11"																																																				
10"																																																				
Width																																																				

Depth	22"	C-C-10W22D	C-C-11W22D	C-C-12W22D	C-C-13W22D	C-C-14W22D	C-C-15W22D	C-C-16W22D	C-C-17W22D	C-C-18W22D	C-C-19W22D	C-C-20W22D	C-C-21W22D	C-C-22W22D	C-C-23W22D	C-C-24W22D	C-C-25W22D	C-C-26W22D	C-C-27W22D	C-C-28W22D
	21"	C-C-10W21D	C-C-11W21D	C-C-12W21D	C-C-13W21D	C-C-14W21D	C-C-15W21D	C-C-16W21D	C-C-17W21D	C-C-18W21D	C-C-19W21D	C-C-20W21D	C-C-21W21D	C-C-22W21D	C-C-23W21D	C-C-24W21D	C-C-25W21D	C-C-26W21D	C-C-27W21D	C-C-28W21D
	20"	C-C-10W20D	C-C-11W20D	C-C-12W20D	C-C-13W20D	C-C-14W20D	C-C-15W20D	C-C-16W20D	C-C-17W20D	C-C-18W20D	C-C-19W20D	C-C-20W20D	C-C-21W20D	C-C-22W20D	C-C-23W20D	C-C-24W20D	C-C-25W20D	C-C-26W20D	C-C-27W20D	C-C-28W20D
	19"	C-C-10W19D	C-C-11W19D	C-C-12W19D	C-C-13W19D	C-C-14W19D	C-C-15W19D	C-C-16W19D	C-C-17W19D	C-C-18W19D	C-C-19W19D	C-C-20W19D	C-C-21W19D	C-C-22W19D	C-C-23W19D	C-C-24W19D	C-C-25W19D	C-C-26W19D	C-C-27W19D	C-C-28W19D
	18"	C-C-10W18D	C-C-11W18D	C-C-12W18D	C-C-13W18D	C-C-14W18D	C-C-15W18D	C-C-16W18D	C-C-17W18D	C-C-18W18D	C-C-19W18D	C-C-20W18D	C-C-21W18D	C-C-22W18D	C-C-23W18D	C-C-24W18D	C-C-25W18D	C-C-26W18D	C-C-27W18D	C-C-28W18D
	17"	C-C-10W17D	C-C-11W17D	C-C-12W17D	C-C-13W17D	C-C-14W17D	C-C-15W17D	C-C-16W17D	C-C-17W17D	C-C-18W17D	C-C-19W17D	C-C-20W17D	C-C-21W17D	C-C-22W17D	C-C-23W17D	C-C-24W17D	C-C-25W17D	C-C-26W17D	C-C-27W17D	C-C-28W17D
	16"	C-C-10W16D	C-C-11W16D	C-C-12W16D	C-C-13W16D	C-C-14W16D	C-C-15W16D	C-C-16W16D	C-C-17W16D	C-C-18W16D	C-C-19W16D	C-C-20W16D	C-C-21W16D	C-C-22W16D	C-C-23W16D	C-C-24W16D	C-C-25W16D	C-C-26W16D	C-C-27W16D	C-C-28W16D
	15"	C-C-10W15D	C-C-11W15D	C-C-12W15D	C-C-13W15D	C-C-14W15D	C-C-15W15D	C-C-16W15D	C-C-17W15D	C-C-18W15D	C-C-19W15D	C-C-20W15D	C-C-21W15D	C-C-22W15D	C-C-23W15D	C-C-24W15D	C-C-25W15D	C-C-26W15D	C-C-27W15D	C-C-28W15D
	14"	C-C-10W14D	C-C-11W14D	C-C-12W14D	C-C-13W14D	C-C-14W14D	C-C-15W14D	C-C-16W14D	C-C-17W14D	C-C-18W14D	C-C-19W14D	C-C-20W14D	C-C-21W14D	C-C-22W14D	C-C-23W14D	C-C-24W14D	C-C-25W14D	C-C-26W14D	C-C-27W14D	C-C-28W14D
	13"	C-C-10W13D	C-C-11W13D	C-C-12W13D	C-C-13W13D	C-C-14W13D	C-C-15W13D	C-C-16W13D	C-C-17W13D	C-C-18W13D	C-C-19W13D	C-C-20W13D	C-C-21W13D	C-C-22W13D	C-C-23W13D	C-C-24W13D	C-C-25W13D	C-C-26W13D	C-C-27W13D	C-C-28W13D
	12"	C-C-10W12D	C-C-11W12D	C-C-12W12D	C-C-13W12D	C-C-14W12D	C-C-15W12D	C-C-16W12D	C-C-17W12D	C-C-18W12D	C-C-19W12D	C-C-20W12D	C-C-21W12D	C-C-22W12D	C-C-23W12D	C-C-24W12D	C-C-25W12D	C-C-26W12D	C-C-27W12D	C-C-28W12D
	11"	C-C-10W11D	C-C-11W11D	C-C-12W11D	C-C-13W11D	C-C-14W11D	C-C-15W11D	C-C-16W11D	C-C-17W11D	C-C-18W11D	C-C-19W11D	C-C-20W11D	C-C-21W11D	C-C-22W11D	C-C-23W11D	C-C-24W11D	C-C-25W11D	C-C-26W11D	C-C-27W11D	C-C-28W11D
	10"	C-C-10W10D	C-C-11W10D	C-C-12W10D	C-C-13W10D	C-C-14W10D	C-C-15W10D	C-C-16W10D	C-C-17W10D	C-C-18W10D	C-C-19W10D	C-C-20W10D	C-C-21W10D	C-C-22W10D	C-C-23W10D	C-C-24W10D	C-C-25W10D	C-C-26W10D	C-C-27W10D	C-C-28W10D
		10"	11"	12"	13"	14"	15"	16"	17"	18"	19"	20"	21"	22"	23"	24"	25"	26"	27"	28"
		Width																		

Phone: 800.736.0925 | Fax: 877.636.8944 | permobil.com

Order #: _____

CD-INCEPTION-FORM REV100322

1 of 12

DO NOT SEND PROTECTED HEALTH INFORMATION. IT IS NOT NEEDED TO MAKE THE PRODUCT YOU ARE REQUESTING.

1.2


Cover material options

MSRP Standard \$0.00 | w/GlideWear \$23.00



COMFORT-TEK®

A smooth, easily cleaned surface. The incontinence protection also aids in infection control.



STRETCH-AIR®

Stretch-Air has comfortable stretch and heat dissipation.

GlideWear™

Shear reduction panel



Selected for shear reduction, micro-climate control and improved comfort. This fabric panel sits below the bony prominences for maximum skin protection.

COMFORT-TEK

Standard

(CD-COMFORT-TEK)

WITH GlideWear

(CD-GW-COMFORT-TEK)

STRETCH-AIR

Standard

(CD-STRETCH-AIR)

WITH GlideWear

(CD-GW-STRETCH-AIR)

1.3

Incontinence liner

MSRP \$80.00

NOTE: If a ROHO Air Insert is selected, Incontinent Liner will have a small opening for the valve hose.

Incontinence Liner (CD-INCON-LINER)

1.4

Extra cover

MSRP Standard \$83.00 | w/GlideWear \$105.00

COMFORT-TEK

Standard

(CD-X-COMFORT-TEK)

WITH GlideWear

(CD-GW-X-COMFORT-TEK)

STRETCH-AIR

Standard

(CD-X-STRETCH-AIR)

WITH GlideWear


(CD-GW-X-STRETCH-AIR)

2 Base specifications

Seat shape reference guide

Linear


- Base Structure - Flat Bottom with ¼" Crosslink
- Lower Layer - 1" HR Medium
- Middle Layer - ½" HR Medium
- Topper Layer - ½" Viscool Soft



Anti-thrust

Foam layers as listed in Linear, PLUS...


- Anti-Thrust - 1" H (15W and above)
½ seat depth or ½" H (14W or below)



Zero elevation contour

Foam layers as listed in Linear, PLUS...


- Straight Adductors - 1 ½" H (15W and above)
or 1" H (14W or below)
- Abductor - 1 ½" H (15W and above)
or 1" H (14W or below)



Anti-thrust contour

Foam layers as listed in Linear, PLUS...

- Anti-Thrust - 1" H (15W and above)
½ seat depth or ½" H (14W or below)
- Straight Adductors - 1 ½" H (15W and above)
or 1" H (14W or below)
- Abductor - 1 ½" H (15W and above)
or 1" H (14W or below)



Order #: _____

CD-INCEPTION-FORM REV100322

"DO NOT SEND PROTECTED HEALTH INFORMATION. IT IS NOT NEEDED TO MAKE THE PRODUCT YOU ARE REQUESTING."

2.1 Bottom style

A.

NOTE: Only **one** bottom style may be selected. Flat Bottom is standard if an alternate style is not selected.

Flat MSRP \$0.00



Front view

Flat bottom (CD-FLAT-BOTTOM)

Round MSRP \$35.00



Front view



Round bottom (CD-ROUND-BOTTOM)

NOTE: If choosing a wedge in subsection A, proceed to subsection B and choose a wedge height.

NOTE: If a round bottom style is selected, 1/2" to 1" of additional profile height will be added to the seat support. Cannot be paired with rigid insert.

NOTE: A reverse wedge will add height to the rear of the seat support surface. Cannot be paired with ROHO Air Insert, only full wedges available with anti-thrust and ischial insert.


Wedge (MSRP notes in height selection)

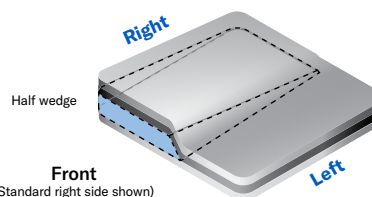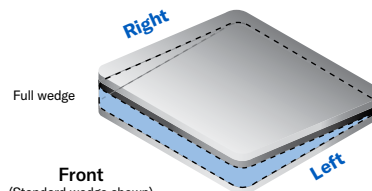

B.

NOTE: Wedge is not a removable feature.

Wedge height MSRP \$35.00

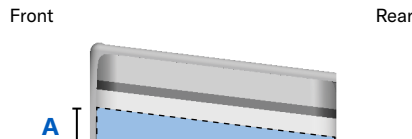

A = 1" (CD-WEDGE-1)

A = 2" (CD-WEDGE-2)

A = 3" (CD-WEDGE-3)

A = Other _____ (CD-WEDGE-OTHER)

Standard full wedge (CD-WEDGE-STANDARD)

Standard left side (CD-WEDGE-LEFT)

Standard right side (CD-WEDGE-RIGHT)

Reverse full wedge (CD-WEDGE-REV)

Reverse left side (CD-WEDGE-REV-LEFT)


Reverse right side (CD-WEDGE-REV-RIGHT)

2.2 Anti-thrust MSRP \$0.00

INSTRUCTIONS: Choose one style and height (directly below your style choice) in subsection A. Anti-thrust will be 1/2 of the seat support depth unless otherwise noted in subsection B. **NOTE:** Depth dimension is determined before growth kit strips are applied. Cannot be paired with a ROHO Air Insert or a left or right wedge.

A.

Anti-thrust style & height



Side view

Standard anti-thrust (CD-AT-STANDARD)

Left side only (CD-AT-LEFT)

Right side only (CD-AT-RIGHT)

B = 1/2" (CD-AT-HEIGHT-0.5)


B = 1" (CD-AT-HEIGHT-1.0)

B = 1 1/2" (CD-AT-HEIGHT-1.5)

B = 2" (CD-AT-HEIGHT-2.0)

B = 2 1/2" (CD-AT-HEIGHT-2.5)

B = Other _____
(CD-AT-HEIGHT-OTHER)



Side view

Standard anti-thrust **with growth kit**
(CD-AT-STND-GROWTH-KIT)

Anti-Thrust with (3) 1" strips included for growing the Anti-Thrust depth. Top layer foam is not glued in the seat well allowing access to the 1" pieces.

B = 1/2" (CD-AT-GK-HEIGHT-0.5)

B = 1" (CD-AT-GK-HEIGHT-1.0)

B = 1 1/2" (CD-AT-GK-HEIGHT-1.5)


B = 2" (CD-AT-GK-HEIGHT-2.0)

B = 2 1/2" (CD-AT-GK-HEIGHT-2.5)

B = Other _____
(CD-AT-GK-HEIGHT-OTHER)

B.

Anti-thrust depth

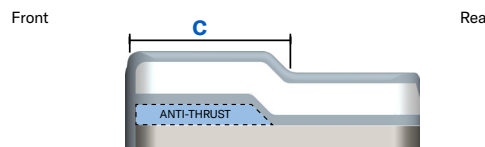

Side view

C = 4" (CD-AT-DEPTH-4)

C = 5" (CD-AT-DEPTH-5)

C = 6" (CD-AT-DEPTH-6)

C = 7" (CD-AT-DEPTH-7)

C = 8" (CD-AT-DEPTH-8)

C = 9" (CD-AT-DEPTH-9)

C = 10" (CD-AT-DEPTH-10)

C = 11" (CD-AT-DEPTH-11)

C = 12" (CD-AT-DEPTH-12)

C = 13" (CD-AT-DEPTH-13)

C = 14" (CD-AT-DEPTH-14)

C = 15" (CD-AT-DEPTH-15)

C = 16" (CD-AT-DEPTH-16)

C = Other _____
(CD-AT-DEPTH-OTHER)

Order #: _____

CD-INCEPTION-FORM REV100322

DO NOT SEND PROTECTED HEALTH INFORMATION. IT IS NOT NEEDED TO MAKE THE PRODUCT YOU ARE REQUESTING.

3 Foam layers

NOTE: If ordering a ROHO Insert, please see Section 4.1 for foam layer restrictions.

Foam recommendations by user weight:

Pediatric or User <100 lbs. (45 kg)		FIRM	HRM	HRS	VIS-M	VIS-S	VIS-XS	VIS-XXS
Lower layer	Minimum 1 ½" (lower and mid layer combined)	●	●		●			
Mid layer			●		●	●		
Topper layer	Minimum ¼"			●		●	●	●

Standard user 100 to 350 lbs. (45-158 kg)		FIRM	HRM	HRS	VIS-M	VIS-S	VIS-XS	VIS-XXS
Lower layer	Minimum 2 ½" (lower and mid layer combined)	●	●		●			
Mid layer			●		●	●		
Topper layer	Minimum ¼"			●		●	●	●

Bariatric user >350 lbs. (158 kg)		FIRM	HRM	HRS	VIS-M	VIS-S	VIS-XS	VIS-XXS
Lower layer	Minimum 3 ½" (lower and mid layer combined)	●	●		●			
Mid layer			●		●	●		
Topper layer	Minimum ½"		●	●	●	●	●	●


3.1 Structural layer

MSRP \$0.00

None	CD-FOAM-STRUCTURAL-NONE	
¼"	Crosslink CD-FOAM-STRUCTURAL-0.25	

3.2 Lower layers

MSRP HR \$0.00 | Visco \$138.00 each | Crosslink Firm \$35.00 each



NOTE: We do not recommend a MEDIUM foam on top of a SOFT foam. "Other" Visco foam layer thicknesses must be in 1/2" increments. *Additional foam layers, if chosen, will be placed on top of the original layer.

Lower layer thickness

	½"	¾"	1"	1 ¼"	Other	3" Max
HR Medium	CD-LOW-HRM-0.25	CD-LOW-HRM-0.50	CD-LOW-HRM-0.75	CD-LOW-HRM-1.00	CD-LOW-HRM-1.25	CD-LOW-HRM-OTHER
Visco Medium		CD-LOW-VIS-M-0.50		CD-LOW-VIS-M-1.00		CD-ADD-LOW-VIS-M-OTHER
Crosslink Firm		CD-LOW-FRM-0.50		CD-LOW-FRM-1.00		


**1/4" lower layer is only to be used in conjunction with 1/4" structural layer.

*Optional - Additional lower layer thickness

	½"	¾"	1"	1 ¼"	OTHER	3" Max
	CD-ADD-LOW-HRM-0.25	CD-ADD-LOW-HRM-0.50	CD-ADD-LOW-HRM-0.75	CD-ADD-LOW-HRM-1.00	CD-ADD-LOW-HRM-1.25	CD-ADD-LOW-HRM-OTHER
		CD-ADD-LOW-VIS-M-0.50		CD-ADD-LOW-VIS-M-1.00		CD-ADD-LOW-VIS-M-OTHER
		CD-ADD-LOW-FRM-0.50		CD-ADD-LOW-FRM-1.00		

3.3 Mid layers

MSRP HR \$0.00 | Visco \$138.00 each



NOTE: A minimum thickness mid layer must be selected if a QuadraGel insert, ischial gel insert, or ischial memory foam insert is chosen. See section 4.1 for specific details. A recess is cut from the mid layer, so if a recess is selected in section 5.4, the mid layer may need to be thicker to allow for enough support in all areas.

Mid layer thickness

	½"	¾"	1"	1 ¼"	Other	2" Max
HR Medium	CD-MID-HRM-0.25	CD-MID-HRM-0.50	CD-MID-HRM-0.75	CD-MID-HRM-1.00	CD-MID-HRM-1.25	CD-MID-HRM-OTHER
HR Soft	CD-MID-HRS-0.25	CD-MID-HRS-0.50	CD-MID-HRS-0.75	CD-MID-HRS-1.00	CD-MID-HRS-1.25	CD-MID-HRS-OTHER
Visco Medium		CD-MID-VIS-M-0.50		CD-MID-VIS-M-1.00		CD-MID-VIS-M-OTHER
Visco Soft		CD-MID-VIS-S-0.50		CD-MID-VIS-S-1.00		CD-MID-VIS-S-OTHER
Visco X-Soft		CD-MID-VIS-XS-0.50		CD-MID-VIS-XS-1.00		CD-MID-VIS-XS-OTHER


*Optional - Additional mid layer thickness

	½"	¾"	1"	1 ¼"	Other	2" Max
	CD-Add-Mid-HRM-0.25	CD-Add-Mid-HRM-0.50	CD-Add-Mid-HRM-0.75	CD-Add-Mid-HRM-1.00	CD-Add-Mid-HRM-1.25	CD-Add-Mid-HRM-OTHER
	CD-Add-Mid-HRS-0.25	CD-Add-Mid-HRS-0.50	CD-Add-Mid-HRS-0.75	CD-Add-Mid-HRS-1.00	CD-Add-Mid-HRS-1.25	CD-Add-Mid-HRS-OTHER
		CD-Add-Mid-VIS-M-0.50		CD-Add-Mid-VIS-M-1.00		CD-Add-Mid-VIS-M-OTHER
		CD-Add-Mid-VIS-S-0.50		CD-Add-Mid-VIS-S-1.00		CD-Add-Mid-VIS-S-OTHER
		CD-Add-Mid-VIS-XS-0.50		CD-Add-Mid-VIS-XS-1.00		CD-Add-Mid-VIS-XS-OTHER

3.4 Topper layers

MSRP HR \$0.00 | Visco \$138.00 each

NOTE: A minimum 1/4" thick topper layer must be selected here if a QuadraGel insert, ischial gel insert, or ischial memory foam insert was chosen in section 4.1.



Topper layer thickness

	½"	¾"	1"	1 ¼"	Other	2" Max
HR Medium	CD-TOP-HRM-0.25	CD-TOP-HRM-0.50	CD-TOP-HRM-0.75	CD-TOP-HRM-1.00	CD-TOP-HRM-1.25	CD-TOP-HRM-OTHER
HR Soft	CD-TOP-HRS-0.25	CD-TOP-HRS-0.50	CD-TOP-HRS-0.75	CD-TOP-HRS-1.00	CD-TOP-HRS-1.25	CD-TOP-HRS-OTHER
Visco Medium		CD-TOP-VIS-M-0.50		CD-TOP-VIS-M-1.00		CD-TOP-VIS-M-OTHER
Visco Soft		CD-TOP-VIS-S-0.50		CD-TOP-VIS-S-1.00		CD-TOP-VIS-S-OTHER
Visco X-Soft		CD-TOP-VIS-XS-0.50		CD-TOP-VIS-XS-1.00		CD-TOP-VIS-XS-OTHER
Visco XX-Soft		CD-TOP-VIS-XXS-0.50		CD-TOP-VIS-XXS-1.00		CD-TOP-VIS-XXS-OTHER

*Optional - Additional topper layer thickness

	½"	¾"	1"	1 ¼"	Other	2" Max
	CD-ADD-TOP-HRM-0.25	CD-ADD-TOP-HRM-0.50	CD-ADD-TOP-HRM-0.75	CD-ADD-TOP-HRM-1.00	CD-ADD-TOP-HRM-1.25	CD-ADD-TOP-HRM-OTHER
	CD-ADD-TOP-HRS-0.25	CD-ADD-TOP-HRS-0.50	CD-ADD-TOP-HRS-0.75	CD-ADD-TOP-HRS-1.00	CD-ADD-TOP-HRS-1.25	CD-ADD-TOP-HRS-OTHER
		CD-ADD-TOP-VIS-M-0.50		CD-ADD-TOP-VIS-M-1.00		CD-ADD-TOP-VIS-M-OTHER
		CD-ADD-TOP-VIS-S-0.50		CD-ADD-TOP-VIS-S-1.00		CD-ADD-TOP-VIS-S-OTHER
		CD-ADD-TOP-VIS-XS-0.50		CD-ADD-TOP-VIS-XS-1.00		CD-ADD-TOP-VIS-XS-OTHER
		CD-ADD-TOP-VIS-XXS-0.50		CD-ADD-TOP-VIS-XXS-1.00		CD-ADD-TOP-VIS-XXS-OTHER

Order #: _____

CD-INCEPTION-FORM REV100322

DO NOT SEND PROTECTED HEALTH INFORMATION. IT IS NOT NEEDED TO MAKE THE PRODUCT YOU ARE REQUESTING.


4 Ischial modifications

4.1 Ischial modifications

NOTE: Ischial inserts are recessed into the mid layer of foam and sit beneath the topper layer. Only **one** insert may be selected. Additional ischial modification options on next page.

NOTE: A minimum of 3/4" mid layer is required for this insert in section 3.3. Cannot be paired with a ROHO Air Insert or left/right wedge.


QuadraGel® insert MSRP \$90.00

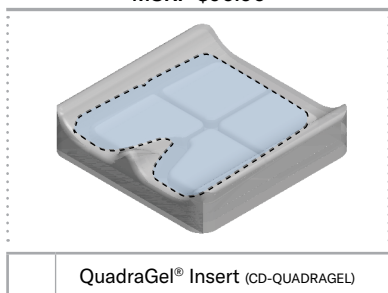

QuadraGel® Insert (CD-QUADRAGEL)

NOTE: A minimum of 1/2" mid layer is required for this insert in section 3.3. Cannot be paired with a ROHO Air Insert or left/right wedge.


Ischial gel insert MSRP \$69.00

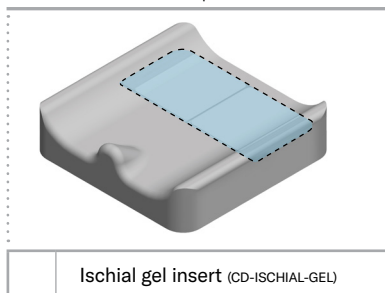

Ischial gel insert (CD-ISCHIAL-GEL)

NOTE: A mid layer of foam must be selected in section 3.3 and, at a minimum, match the insert thickness selected. Cannot be paired with a ROHO Air Insert. Foam type cannot match foam type selected for mid layer in 3.3.


Ischial Visco memory foam insert MSRP \$62.00

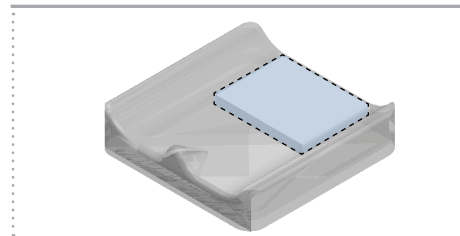

1" thick soft Visco memory foam insert (CD-ISCHIAL-SOFT-1.0)
1" thick x-soft Visco memory foam insert (CD-ISCHIAL-XSOFT-1.0)
1" thick xx-soft Visco memory foam insert (CD-ISCHIAL-XXSOFT-1.0)
1/2" thick soft Visco memory foam insert (CD-ISCHIAL-SOFT-0.5)
1/2" thick x-soft Visco memory foam insert (CD-ISCHIAL-XSOFT-0.5)
1/2" thick xx-soft Visco memory foam insert (CD-ISCHIAL-XXSOFT-0.5)


NOTE: ROHO Air Insert includes hand pump and repair kit.

ROHO® Air Insert MSRP \$375.00

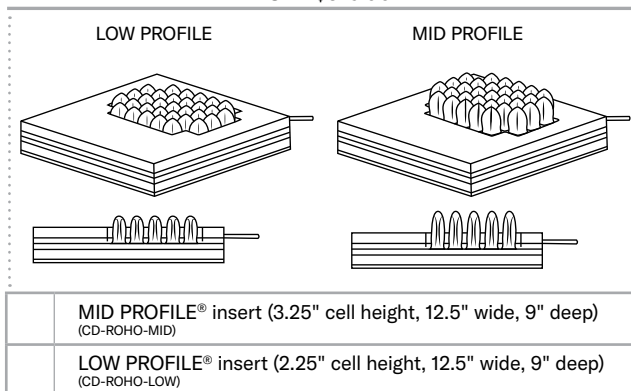

MID PROFILE® insert (3.25" cell height, 12.5" wide, 9" deep)
(CD-ROHO-MID)

LOW PROFILE® insert (2.25" cell height, 12.5" wide, 9" deep)
(CD-ROHO-LOW)

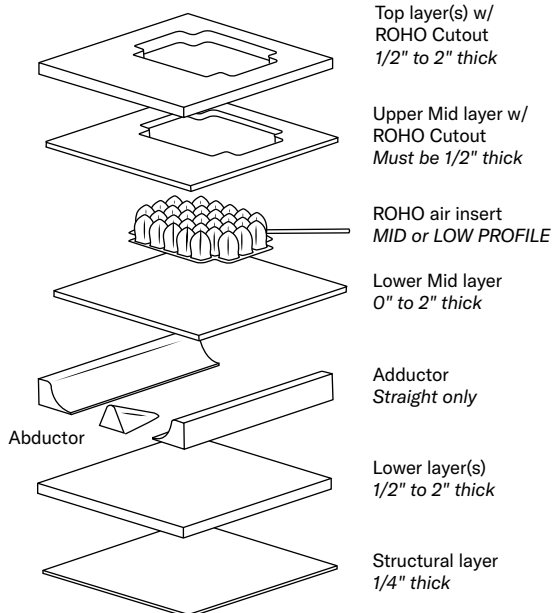

SIZE RESTRICTIONS:

- Minimum width: 16W
- Minimum depth: 16D

FOAM RESTRICTIONS:

- Top layer:
- No HR/Visco Medium foams
- Middle layer:
- Only HR/Visco Medium foams
 - Top mid layer must be 1/2" thick

ROHO INSERT CANNOT BE PAIRED WITH:

- Wedge
- Anti-thrust
- Gel insert or Ischial memory foam insert
- Recess
- Coccyx cut out
- Tapered adductors

Can be paired with Straight adductors if seat is 18W or greater.

5 Custom specs & geometry


5.1 Adduction

INSTRUCTIONS: Select an adductor height for each side in subsection A, select an adductor style and material for each side in subsection B. If no adduction is needed, choose "none" in subsection A.

If a height is selected but not a style, a full-length, straight, adductor will be applied.

NOTE: Custom adductor requests should be noted in the "Additional information" section 9.1.

NOTE: In subsection B, one adductor style may be selected for each side of the seat support. Front or rear only adductor will be 1/2 the seat support depth or match an anti-thrust depth. Tapered adductor cannot be paired with ROHO Air Insert. Straight adductor CAN be paired with a ROHO Air Insert, but must have a seat width 18 wide or greater.



Tapered Adductor Shape
Straight Adductor Shape
REAR ONLY Adduction Area
FRONT ONLY Adduction Area

A.

D	Left adductor height
D = 1/2" (CD-LEFT-ADD-0.5)	
D = 1" (CD-LEFT-ADD-1.0)	
D = 1 1/2" (Standard) (CD-LEFT-ADD-1.5)	
D = 2" (CD-LEFT-ADD-2.0)	
D = 2 1/2" (CD-LEFT-ADD-2.5)	
D = Other _____ (CD-LEFT-ADD-OTHER)	

B.

	Left adductor style
	Tapered adductor, HR Medium (CD-LEFT-ADD-TAPERED)
	Straight adductor, HR Medium (CD-LEFT-ADD-STRAIGHT)
	Rear only straight adductor, HR Medium (CD-LEFT-ADD-REAR-ONLY)
	Front only straight adductor, HR Medium (CD-LEFT-ADD-FRONT-ONLY)
	Tapered adductor, Crosslink Firm (CD-LEFT-ADD-TAPERED-FIRM)
	Straight adductor, Crosslink Firm (CD-LEFT-ADD-STRAIGHT-FIRM)
	Rear only straight adductor, Crosslink Firm (CD-LEFT-ADD-REAR-ONLY-FIRM)
	Front only straight adductor, Crosslink Firm (CD-LEFT-ADD-FRONT-ONLY-FIRM)

C.

	No adductor
	None (CD-LEFT-ADD-NONE)

Rear view

MSRP None/HR Medium \$0.00 | Crosslink Firm \$35.00

E	Right adductor height
E = 1/2" (CD-RIGHT-ADD-0.5)	
E = 1" (CD-RIGHT-ADD-1.0)	
E = 1 1/2" (Standard) (CD-RIGHT-ADD-1.5)	
E = 2" (CD-RIGHT-ADD-2.0)	
E = 2 1/2" (CD-RIGHT-ADD-2.5)	
E = Other _____ (CD-RIGHT-ADD-OTHER)	

	Right adductor style
	Tapered adductor, HR Medium (CD-RIGHT-ADD-TAPERED)
	Straight adductor, HR Medium (CD-RIGHT-ADD-STRAIGHT)
	Rear only straight adductor, HR Medium (CD-RIGHT-ADD-REAR-ONLY)
	Front only straight adductor, HR Medium (CD-RIGHT-ADD-FRONT-ONLY)
	Tapered adductor, Crosslink Firm (CD-RIGHT-ADD-TAPERED-FIRM)
	Straight adductor, Crosslink Firm (CD-RIGHT-ADD-STRAIGHT-FIRM)
	Rear only straight adductor, Crosslink Firm (CD-RIGHT-ADD-REAR-ONLY-FIRM)
	Front only straight adductor, Crosslink Firm (CD-RIGHT-ADD-FRONT-ONLY-FIRM)

	No adductor
	None (CD-RIGHT-ADD-NONE)


5.2 Abduction

MSRP None/HR Medium \$0.00 | Crosslink Firm \$35.00

INSTRUCTIONS: Select an abductor height and an abductor material.

NOTE: Custom abductor requests should be noted in the "Additional information" section 9.1.

Abductor height and material




Front view

None (CD-ABD-NONE)	F = 1/2", Crosslink Firm (CD-ABD-HEIGHT-0.5-FIRM)
F = 1/2", HR Medium (CD-ABD-HEIGHT-0.5)	F = 1", Crosslink Firm (CD-ABD-HEIGHT-1.0-FIRM)
F = 1", HR Medium (CD-ABD-HEIGHT-1.0)	F = 1 1/2", Crosslink Firm (CD-ABD-HEIGHT-1.5-FIRM)
F = 1 1/2", HR Medium (CD-ABD-HEIGHT-1.5)	F = 2", Crosslink Firm (CD-ABD-HEIGHT-2.0-FIRM)
F = 2", HR Medium (CD-ABD-HEIGHT-2.0)	F = 2 1/2", Crosslink Firm (CD-ABD-HEIGHT-2.5-FIRM)
F = 2 1/2", HR Medium (CD-ABD-HEIGHT-2.5)	F = Other, Crosslink Firm _____ (CD-ABD-HEIGHT-OTHER-FIRM)
F = Other, HR Medium _____ (CD-ABD-HEIGHT-OTHER)	

5.3 Coccyx cut out

MSRP \$0.00

NOTE: Coccyx cut out will be centered and cut in the lower layer of foam. If gel insert is selected, additional mid layer is required. Cannot be paired with ROHO Air Insert. Cannot be paired with a recess in section 5.5. Custom cut out requests should be noted in the "Additional information" section 9.1.

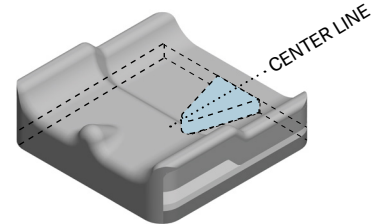

Coccyx Cut Out (CD-COCYX-CUT)

Order #: _____

CD-INCEPTION-FORM REV100322

"DO NOT SEND PROTECTED HEALTH INFORMATION. IT IS NOT NEEDED TO MAKE THE PRODUCT YOU ARE REQUESTING."

6 of 12

5.4

Recess


MSRP \$158.00

NOTE: If a recess is selected, the mid layer foam thickness in section 3.3 must match the TOTAL amount of modifications selected in 4.1 and 5.2. Cannot be paired with ROHO Air Insert or coccyx cutout.

Rear quadrant recess



Front



Front

L	Left side	R	Right side
	1/4" H (CD-IR-LEFT-REAR-0.25)		1/4" H (CD-IR-RIGHT-REAR-0.25)
	1/2" H (CD-IR-LEFT-REAR-0.5)		1/2" H (CD-IR-RIGHT-REAR-0.5)
	3/4" H (CD-IR-LEFT-REAR-0.75)		3/4" H (CD-IR-RIGHT-REAR-0.75)
	1" H (CD-IR-LEFT-REAR-1.0)		1" H (CD-IR-RIGHT-REAR-1.0)
	1 1/4" H (CD-IR-LEFT-REAR-1.25)		1 1/4" H (CD-IR-RIGHT-REAR-1.25)
	Other _____ (CD-IR-LEFT-REAR-OTHER)		Other _____ (CD-IR-RIGHT-REAR-OTHER)

Full length recess



Front




Front

L	Left side	R	Right side
	1/4" H (CD-IR-LEFT-FULL-0.25)		1/4" H (CD-IR-RIGHT-FULL-0.25)
	1/2" H (CD-IR-LEFT-FULL-0.5)		1/2" H (CD-IR-RIGHT-FULL-0.5)
	3/4" H (CD-IR-LEFT-FULL-0.75)		3/4" H (CD-IR-RIGHT-FULL-0.75)
	1" H (CD-IR-LEFT-FULL-1.0)		1" H (CD-IR-RIGHT-FULL-1.0)
	1 1/4" H (CD-IR-LEFT-FULL-1.25)		1 1/4" H (CD-IR-RIGHT-FULL-1.25)
	Other _____ (CD-IR-LEFT-FULL-OTHER)		Other _____ (CD-IR-RIGHT-FULL-OTHER)

5.5


Hamstring relief

MSRP \$35.00



NOTE: Choose one hamstring relief option. Left or right side relief will be half the width of the cushion. Custom requests should be noted in "Additional information" section 9.1.


Full width relief



Front

G	= 1" D (CD-HAM-RELIEF-1)
G	= 2" D (CD-HAM-RELIEF-2)
G	= Other _____ (CD-HAM-RELIEF-OTHER)


Left side relief



Front

G	= 1" D (CD-LEFT-HAM-RELIEF-1)
G	= 2" D (CD-LEFT-HAM-RELIEF-2)
G	= Other _____ (CD-LEFT-HAM-RELIEF-OTHER)

Right side relief



Front

G	= 1" D (CD-RIGHT-HAM-RELIEF-1)
G	= 2" D (CD-RIGHT-HAM-RELIEF-2)
G	= Other _____ (CD-RIGHT-HAM-RELIEF-OTHER)


5.6

Growth notches

MSRP \$35.00

NOTE: Growth notches may affect any adductors at the rear of the seat support. *Tip: An anti-thrust growth kit from section 2.2 subsection A can be used to adjust the seat well depth as well, if an anti-thrust feature is needed.*

Depth of notches

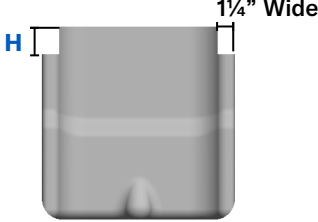

Top view

H	= 1" D (CD-GROWTH-NOTCH-1)
H	= 2" D (CD-GROWTH-NOTCH-2)
H	= 3" D (CD-GROWTH-NOTCH-3)
H	= Other _____ (CD-GROWTH-NOTCH-OTHER)

5.7

Rail cuts

MSRP \$35.00

NOTE: Rail cuts will affect how much cushion is left along the sides of especially low-profile seat supports. Cannot be paired with Removable Solid Seat Pan or ATI.

Rail cut height



Front view

J	= 1" Rail cut (CD-RAIL-CUT-1.0)
J	= 1 1/2" Rail cut (CD-RAIL-CUT-1.5)
J	= 2" Rail cut (CD-RAIL-CUT-2.0)
J	= Other _____ (CD-RAIL-CUT-OTHER)


5.8

Leg length discrepancy

MSRP \$103.00


NOTE: Offset discrepancy maintains foam abductor shape and removable abductor placement.

Standard leg length discrepancy

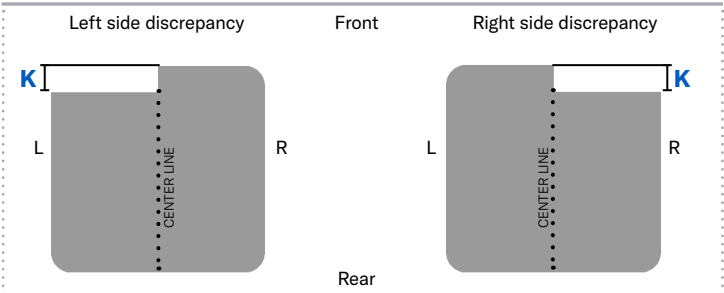

L	Depth removed from side		R
(CD-LLD-DEPTH-L-0.5)	$K = \frac{1}{2}" D$	(CD-LLD-DEPTH-R-0.5)	
(CD-LLD-DEPTH-L-1.0)	$K = 1" D$	(CD-LLD-DEPTH-R-1.0)	
(CD-LLD-DEPTH-L-1.5)	$K = 1\frac{1}{2}" D$	(CD-LLD-DEPTH-R-1.5)	
(CD-LLD-DEPTH-L-2.0)	$K = 2" D$	(CD-LLD-DEPTH-R-2.0)	
(CD-LLD-DEPTH-L-OTHER)	$K = \text{Other } \underline{\hspace{1cm}}$	(CD-LLD-DEPTH-R-OTHER)	

Offset leg length discrepancy

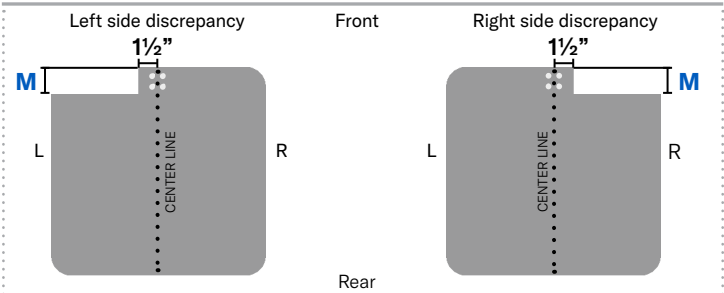

L	Depth removed from side		R
(CD-LLD-O-DEPTH-L-0.5)	$M = \frac{1}{2}" D$	(CD-LLD-O-DEPTH-R-0.5)	
(CD-LLD-O-DEPTH-L-1.0)	$M = 1" D$	(CD-LLD-O-DEPTH-R-1.0)	
(CD-LLD-O-DEPTH-L-1.5)	$M = 1\frac{1}{2}" D$	(CD-LLD-O-DEPTH-R-1.5)	
(CD-LLD-O-DEPTH-L-2.0)	$M = 2" D$	(CD-LLD-O-DEPTH-R-2.0)	
(CD-LLD-O-DEPTH-L-OTHER)	$M = \text{Other } \underline{\hspace{1cm}}$	(CD-LLD-O-DEPTH-R-OTHER)	

5.9

Platform

MSRP \$515.00

5.10


Insert

NOTE: Accommodates 7/8" or 1" tubing. Comes with two different cross bars to accommodate various wheelchair frame types. Fits both folding and non-folding seat rails. Lateral pelvic/thigh support hardware can be easily attached. Cannot be paired with rail cut. Leg length discrepancy offset maintains centered removable abductor hardware attachment.

NOTE: Moldable ATI (Adjustable Technology Insert for Positioning) enables on-site customization to the contour of the seat support surface. 1/4" Crosslink is not recommended with the ATI. Cannot be paired with rail cuts.


NOTE: Cannot be paired with the round bottom in section 2.1.

Removable solid seat pan

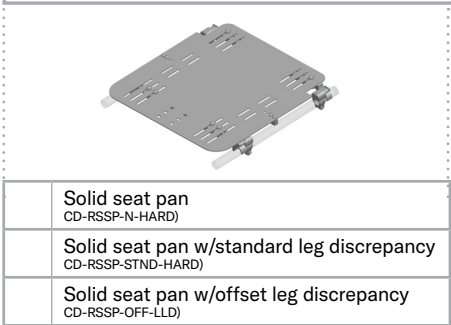


Moldable ATI

MSRP \$193.00

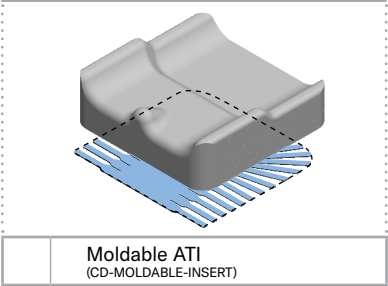


Rigid insert

MSRP \$84.00

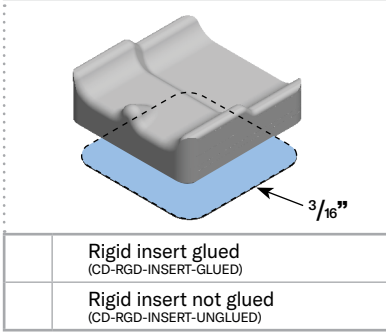

6 Cover accessories

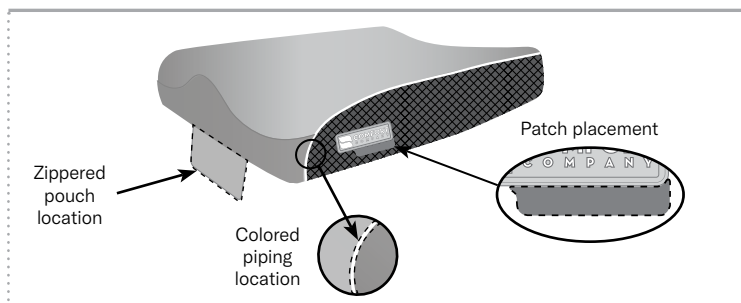

6.1 Military branch patch MSRP \$0.00

Air Force (CD-AIR-FORCE-PATCH)	Marines (CD-MARINES-PATCH)
Army (CD-ARMY-PATCH)	Navy (CD-NAVY-PATCH)

6.2 Zippered pouch MSRP \$35.00

Zippered pouch (CD-ZIP-POUCH)

6.3 Colored piping MSRP \$0.00

NOTE: If no color is selected, our standard silver reflective piping will be used.

Red (CD-RED)	Blue (CD-BLUE)
Purple (CD-PURPLE)	Green (CD-GREEN)
Pink (CD-PINK)	Remove (CD-REMOVE)
Orange (CD-ORANGE)	

7 BodiLink® Lateral Pelvic/Thigh Support hardware & pads

7.1 Premium pad size & shape HCPCS Code: E0953 MSRP \$66.00

- You may make one selection per column (left, extra left, right, and extra right) in section 7.1.
- Make a fabric selection in 7.2.

*Length (L) refers to the actual size dimension of the support from top to bottom edge. Depth (D) refers to the actual size dimension from anterior to posterior edge.

Style	Size	Left	Extra left	Right	Extra right
	3.5"L x 4"D	BL-LPTSP2Z-3L4D-LH	BL-LPTSP2Z-3L4D-LH	BL-LPTSP2Z-3L4D-RH	BL-LPTSP2Z-3L4D-RH
	3.5"L x 8"D	BL-LPTSP2Z-3L8D-LH	BL-LPTSP2Z-3L8D-LH	BL-LPTSP2Z-3L8D-RH	BL-LPTSP2Z-3L8D-RH
	3.5"L x 12"D	BL-LPTSP2Z-3L12D-LH	BL-LPTSP2Z-3L12D-LH	BL-LPTSP2Z-3L12D-RH	BL-LPTSP2Z-3L12D-RH
	5.5"L x 6"D	BL-LPTSP2Z-5L6D-LH	BL-LPTSP2Z-5L6D-LH	BL-LPTSP2Z-5L6D-RH	BL-LPTSP2Z-5L6D-RH

7.2 Premium pad cover with foam insert

Cover options	MSRP	Left	Extra left	Right	Extra right
COMFORT-TEK	\$0.00/ea.	LPTS-P2-COMFORT-FM	LPTS-P2-COMFORT-FM	LPTS-P2-COMFORT-FM	LPTS-P2-COMFORT-FM
STRETCH-AIR	\$0.00/ea.	LPTS-P2-STRETCH-FM	LPTS-P2-STRETCH-FM	LPTS-P2-STRETCH-FM	LPTS-P2-STRETCH-FM
GlideWear	\$13.00/ea.	LPTS-P2-GLIDE-FM	LPTS-P2-GLIDE-FM	LPTS-P2-GLIDE-FM	LPTS-P2-GLIDE-FM



COMFORT-TEK
FOR FLUID PROTECTION & AN
EASILY CLEANED SURFACE.



STRETCH-AIR
FOR PATIENT COMFORT &
HEAT DISSIPATION.



GlideWear
FOR SKIN PROTECTION
& SHEAR REDUCTION.
NOT FLUID RESISTANT.

BodiLink Lateral Pelvic/Thigh Support hardware

- You may make one selection per column (left, extra left, right, and extra right) in section 7.3 from subsection A or B.
- TT long extension arms (section 7.4) will only work with TT style hardware.

A. TT Hardware, Slot mount


TT HARDWARE
SLOT MOUNT- FIXED



TT HARDWARE
SLOT MOUNT- REMOVABLE



HARDWARE SIZE
VS. CUSHION THICKNESS

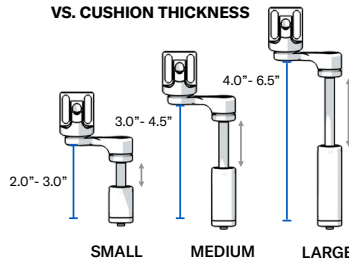


HARDWARE SIZE	MAX CUSHION THICKNESS CLEARANCE	RECOMMENDED CUSHION THICKNESS
SMALL	3.0"	2.0"- 3.0"
MEDIUM	4.5"	3.0"- 4.5"
LARGE	6.5"	4.0"- 6.5"


Size		MSRP	Left		Extra left		Right		Extra right	
FIXED	Small	\$149.00		BL-LPTS-TT1FXSL1-LH		BL-LPTS-TT1FXSL1-LH		BL-LPTS-TT1FXSL1-RH		BL-LPTS-TT1FXSL1-RH
	Medium	\$149.00		BL-LPTS-TT1FXSL2-LH		BL-LPTS-TT1FXSL2-LH		BL-LPTS-TT1FXSL2-RH		BL-LPTS-TT1FXSL2-RH
	Large	\$149.00		BL-LPTS-TT1FXSL3-LH		BL-LPTS-TT1FXSL3-LH		BL-LPTS-TT1FXSL3-RH		BL-LPTS-TT1FXSL3-RH
OR REMOVABLE E1028	Small	\$261.00		BL-LPTS-TT1RMSL1-LH		BL-LPTS-TT1RMSL1-LH		BL-LPTS-TT1RMSL1-RH		BL-LPTS-TT1RMSL1-RH
	Medium	\$261.00		BL-LPTS-TT1RMSL2-LH		BL-LPTS-TT1RMSL2-LH		BL-LPTS-TT1RMSL2-RH		BL-LPTS-TT1RMSL2-RH
	Large	\$261.00		BL-LPTS-TT1RMSL3-LH		BL-LPTS-TT1RMSL3-LH		BL-LPTS-TT1RMSL3-RH		BL-LPTS-TT1RMSL3-RH

B. TT Hardware, Power mount


TT HARDWARE
POWER MOUNT- FIXED



TT HARDWARE
POWER MOUNT- REMOVABLE



HARDWARE SIZE
VS. CUSHION THICKNESS

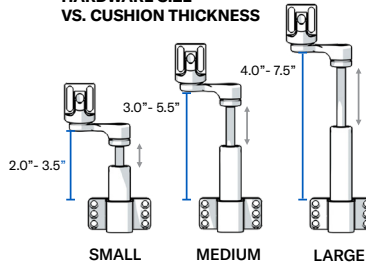

HARDWARE SIZE	MAX CUSHION THICKNESS CLEARANCE	RECOMMENDED CUSHION THICKNESS
SMALL	3.5"	2.0"- 3.5"
MEDIUM	5.5"	3.0"- 5.5"
LARGE	7.5"	4.0"- 7.5"


FIXED	Size	MSRP	Left		Extra left		Right		Extra right	
	Small	\$195.00		BL-LPTS-TT1FXPWL1-LH		BL-LPTS-TT1FXPWL1-LH		BL-LPTS-TT1FXPWL1-RH		BL-LPTS-TT1FXPWL1-RH
	Medium	\$195.00		BL-LPTS-TT1FXPWL2-LH		BL-LPTS-TT1FXPWL2-LH		BL-LPTS-TT1FXPWL2-RH		BL-LPTS-TT1FXPWL2-RH
	Large	\$195.00		BL-LPTS-TT1FXPWL3-LH		BL-LPTS-TT1FXPWL3-LH		BL-LPTS-TT1FXPWL3-RH		BL-LPTS-TT1FXPWL3-RH
OR REMOVABLE E1028	Small	\$300.00		BL-LPTS-TT1RMPWL1-LH		BL-LPTS-TT1RMPWL1-LH		BL-LPTS-TT1RMPWL1-RH		BL-LPTS-TT1RMPWL1-RH
	Medium	\$300.00		BL-LPTS-TT1RMPWL2-LH		BL-LPTS-TT1RMPWL2-LH		BL-LPTS-TT1RMPWL2-RH		BL-LPTS-TT1RMPWL2-RH
	Large	\$300.00		BL-LPTS-TT1RMPWL3-LH		BL-LPTS-TT1RMPWL3-LH		BL-LPTS-TT1RMPWL3-RH		BL-LPTS-TT1RMPWL3-RH

TT Hardware, Power mount option

NOTE: If choosing the power mount hardware, choose the appropriate power mount type below.

Power mount	MSRP	Part number
Quantum	add \$0.00	LPTS-TT1-PW1
Permobil	add \$0.00	LPTS-TT1-PW2
Quickie	add \$0.00	LPTS-TT1-PW3
Rovi	add \$0.00	LPTS-TT1-PW4
Avid Rehab	add \$0.00	LPTS-TT1-PW5

TT Long extension arm 4" MSRP \$39.00/arm



Left	Extra left	Right	Extra right
BL-LPTS-TT1LARM4	BL-LPTS-TT1LARM4	BL-LPTS-TT1LARM4	BL-LPTS-TT1LARM4



8 BodiLink Medial Knee/Thigh Support hardware & pads

- You may make one selection per column.
- Choose between wedge or oval in 8.1.
- Choose a cover material in 8.2.
- Choose hardware size in 8.3.

8.1 Pad size & shape

HCPCS CODING: E0957

MSRP \$137.00

Style	Size	Part number
 WEDGE	2.5"W x 3.5"D	BL-MKTSP1-3W4D
	3.5"W x 5"D	BL-MKTSP1-4W5D
	4"W x 6"D	BL-MKTSP1-4W6D
 OVAL	2.5"W x 3.5"D	BL-MKTSP2-3W4D
	3.5"W x 5"D	BL-MKTSP2-4W5D
	5"W x 6"D	BL-MKTSP2-5W6D

8.2 Pad cover material

GlideWear
INNOVATIVE SKIN PROTECTION

FOR SKIN PROTECTION
& SHEAR REDUCTION.
NOT FLUID RESISTANT.

COMFORT-TEK



FOR FLUID PROTECTION
& AN EASILY CLEANED
SURFACE.

STRETCH-AIR




FOR PATIENT COMFORT
& HEAT DISSIPATION.

	GlideWear (MKTSP-GLIDE) (add \$15.00)
	COMFORT-TEK (MKTSP-COMFORT)
	STRETCH-AIR (MKTSP-STRETCH)

8.3 Medial Knee/Thigh Support swing-away hardware

HCPCS CODING: E1028



MSRP \$189.00



Size	Part number
Small	BL-MKTS-ST1SASL1
Medium	BL-MKTS-ST1SASL2
Large	BL-MKTS-ST1SASL3

*Swing Away Hardware only, not available in Fixed Hardware

**MKTS Hardware must be mounted to Removable Solid Seat Pan in section 4.10.

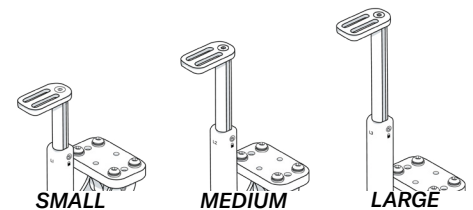

SIZE	RECOMMENDED INFERIOR THIGH THICKNESS
Small	1.00" - 3.00"
Medium	2.00" - 5.00"
Large	3.00" - 7.00"

9 Additional information

9.1 Comments

INSTRUCTIONS: Please reference any section or subsection of the form when making any comments.

Section #	Page #	Comments

INSTRUCTIONS: If preferred, please sketch ideas in the spaces provided below.

SUBMIT BY EMAIL

Order #: _____

CD-INCEPTION-FORM REV100322

DO NOT SEND PROTECTED HEALTH INFORMATION. IT IS NOT NEEDED TO MAKE THE PRODUCT YOU ARE REQUESTING.

12 of 12