


Smart Check[®] Optional Setup Instructions


Optional Setup is an alternative to Smart Setup that records your preferred cushion inflation setting. See OVERVIEW for more information.

Part One: Adjust Your Cushion Without Smart Check

1. Perform a Hard Reset. See HARD RESET INSTRUCTIONS.
NOTE: For first-time use, remove the battery pull tab.
2. Inflate the cushion and place it in the chair. Sit on the cushion in your usual position. Adjust the cushion by following the CUSHION ADJUSTMENT instructions in the *ROHO[®] Single Compartment Cushion with Sensor Ready™ Technology Operation Manual* or the *ROHO[®] Hybrid Elite[®] Cushion Operation Manual*.
3. Perform a hand check to confirm immersion and envelopment. (See the HAND CHECK GUIDE in this manual.)






Symbols and Lights for Optional Setup

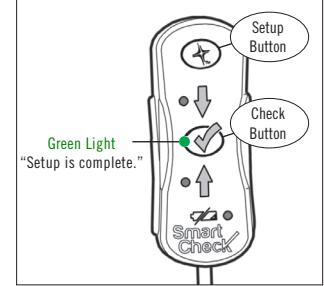

Part Two: Save your Setting with Smart Check



- It is recommended that a qualified seating specialist be consulted when saving a preferred cushion inflation setting with Optional Setup.
- Perform the following steps in the usual environmental conditions.



4. Make sure Smart Check is attached to your cushion. You will hear a “click” when the connection is secure.
5. Make sure the inflation valve is closed. Press the Check ✓ Button to activate Smart Check. You will see either a ↑ or a ↓ red light. **DO NOT** add or remove air.
6. Press and hold the Setup Button for four (4) seconds until you see a green light. The green light means that your preferred cushion inflation setting has been saved. The green light DOES NOT indicate a *Proper Cushion Inflation Setting*. See OVERVIEW for more information.





Store Smart Check in a safe and accessible location. See DISCONNECTION AND STORAGE INSTRUCTIONS.

Your cushion is now set up. (Next: See CHECK INSTRUCTIONS.)

Hand Check Guide

Use this guide to adjust your cushion during Optional Setup. A hand check is also recommended after performing Smart Setup so you will have a reference point if you need to adjust your cushion without Smart Check (for example, if the device has been misplaced).



Before you perform a hand check, refer to IMPORTANT SAFETY INFORMATION and read the warning about using an under-inflated cushion or an over-inflated cushion.



Make sure that there is at least a 1/2 in. (1.5 cm) of air supporting the individual's bony prominences.

1. Place your hand between yourself and the cushion. Feel for the lowest bony prominence. You should be able to slightly move your fingertips.
2. If it feels like the cushion has too much air or not enough air, adjust as needed and see CHECK INSTRUCTIONS and OVERVIEW.